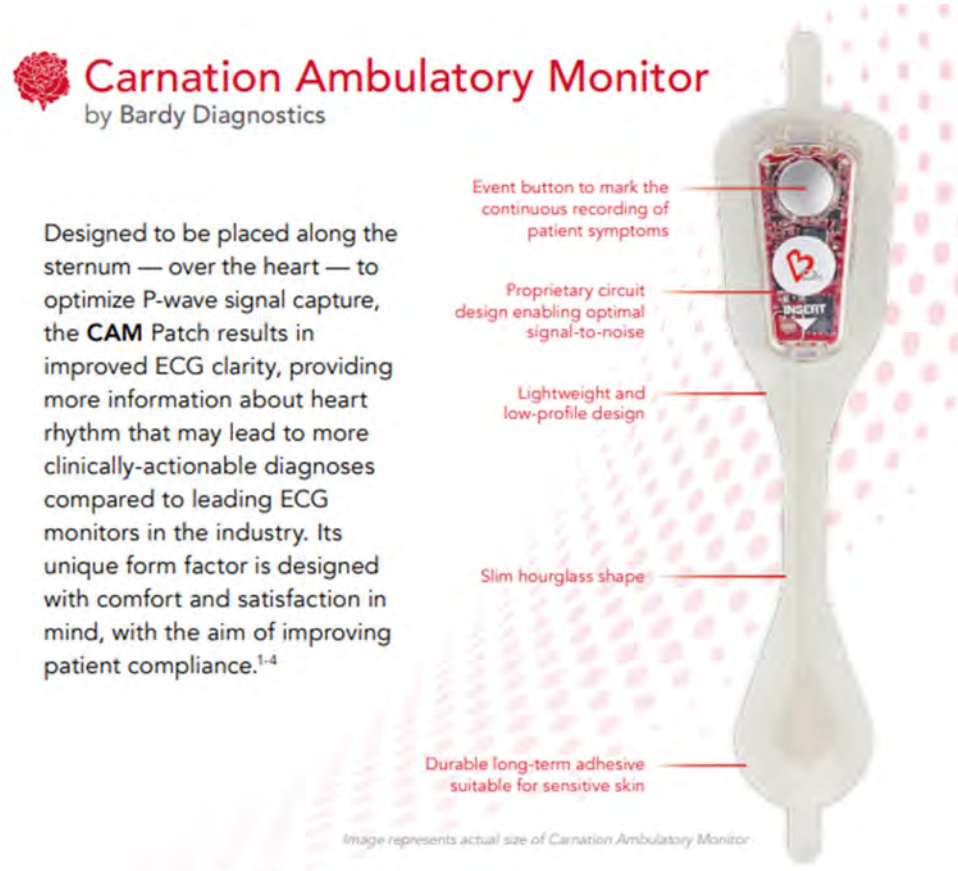
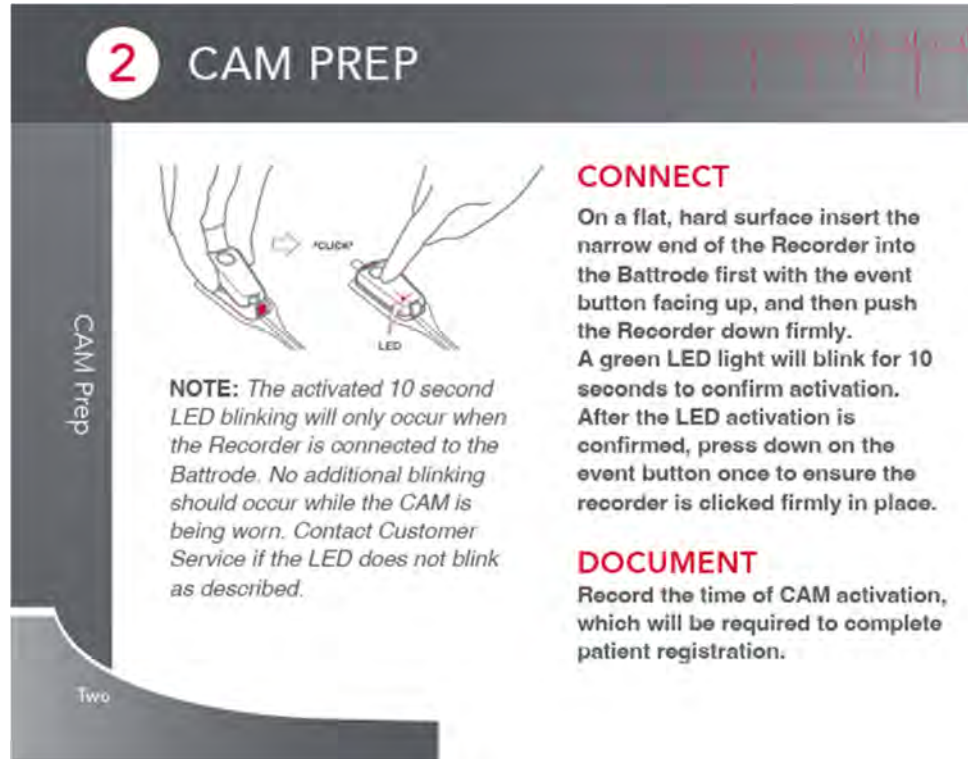


EXHIBIT 14

**Infringement of U.S. Patent No. 12,245,860
By the Bardy CAM Patch Product**


Claim 1	Accused Product
<p>[1.pre] A physiological monitoring device configured to monitor cardiac rhythm data of a patient, the physiological monitoring device comprising:</p>	<p>To the extent the preamble is limiting, the Bardy CAM Patch product comprises a physiological monitoring device configured to monitor cardiac rhythm data of a patient, the physiological monitoring device comprising.</p> <p>The Bardy CAM Patch product comprises a physiological monitoring device configured to monitor cardiac rhythm data of a patient, including, for example, “heart rhythm” and “P-Wave signal capture.”</p> <div data-bbox="581 498 1533 1365">  <p>Carnation Ambulatory Monitor by Bardy Diagnostics</p> <p>Designed to be placed along the sternum — over the heart — to optimize P-wave signal capture, the CAM Patch results in improved ECG clarity, providing more information about heart rhythm that may lead to more clinically-actionable diagnoses compared to leading ECG monitors in the industry. Its unique form factor is designed with comfort and satisfaction in mind, with the aim of improving patient compliance.¹⁻⁴</p> <ul style="list-style-type: none"> Event button to mark the continuous recording of patient symptoms Proprietary circuit design enabling optimal signal-to-noise Lightweight and low-profile design Slim hourglass shape Durable long-term adhesive suitable for sensitive skin <p><small>Image represents actual size of Carnation Ambulatory Monitor</small></p> </div>

**Infringement of U.S. Patent No. 12,245,860
By the Bardy CAM Patch Product**

	<p>(https://www.bardydx.com/wp-content/uploads/2022/12/DN000601A-14Day-Half-fold-CAM-Brochure.pdf)</p>
<p>[1.a] a spring contact configured to electrically couple a battery to a circuit board assembly housed within a first housing portion;</p>	<p>The Bardy CAM Patch product comprises a spring contact configured to electrically couple a battery to a circuit board assembly housed within a first housing portion.</p> <p>For example, the second housing portion, which Bardy calls a Battrode, of the Bardy CAM Patch product comprises a spring contact configured to electrically couple a battery in the Battrode to a circuit board assembly in the first housing portion, which Bardy calls a Recorder, when the housing portions are attached to each other.</p> <div data-bbox="550 599 1512 1354"><p>The image is a page from a brochure titled "2 CAM PREP". It features a diagram showing a hand inserting a "Recorder" into a "Battrode". The Recorder has a red LED light. The Battrode has a spring contact. The diagram is labeled "CONNECT".</p><p>NOTE: The activated 10 second LED blinking will only occur when the Recorder is connected to the Battrode. No additional blinking should occur while the CAM is being worn. Contact Customer Service if the LED does not blink as described.</p><p>CONNECT</p><p>On a flat, hard surface insert the narrow end of the Recorder into the Battrode first with the event button facing up, and then push the Recorder down firmly. A green LED light will blink for 10 seconds to confirm activation. After the LED activation is confirmed, press down on the event button once to ensure the recorder is clicked firmly in place.</p><p>DOCUMENT</p><p>Record the time of CAM activation, which will be required to complete patient registration.</p></div>

**Infringement of U.S. Patent No. 12,245,860
By the Bardy CAM Patch Product**

(https://www.bardydex.com/wp-content/uploads/2023/06/DWG000782B_CAM-Quick-Ref-Guide.pdf)

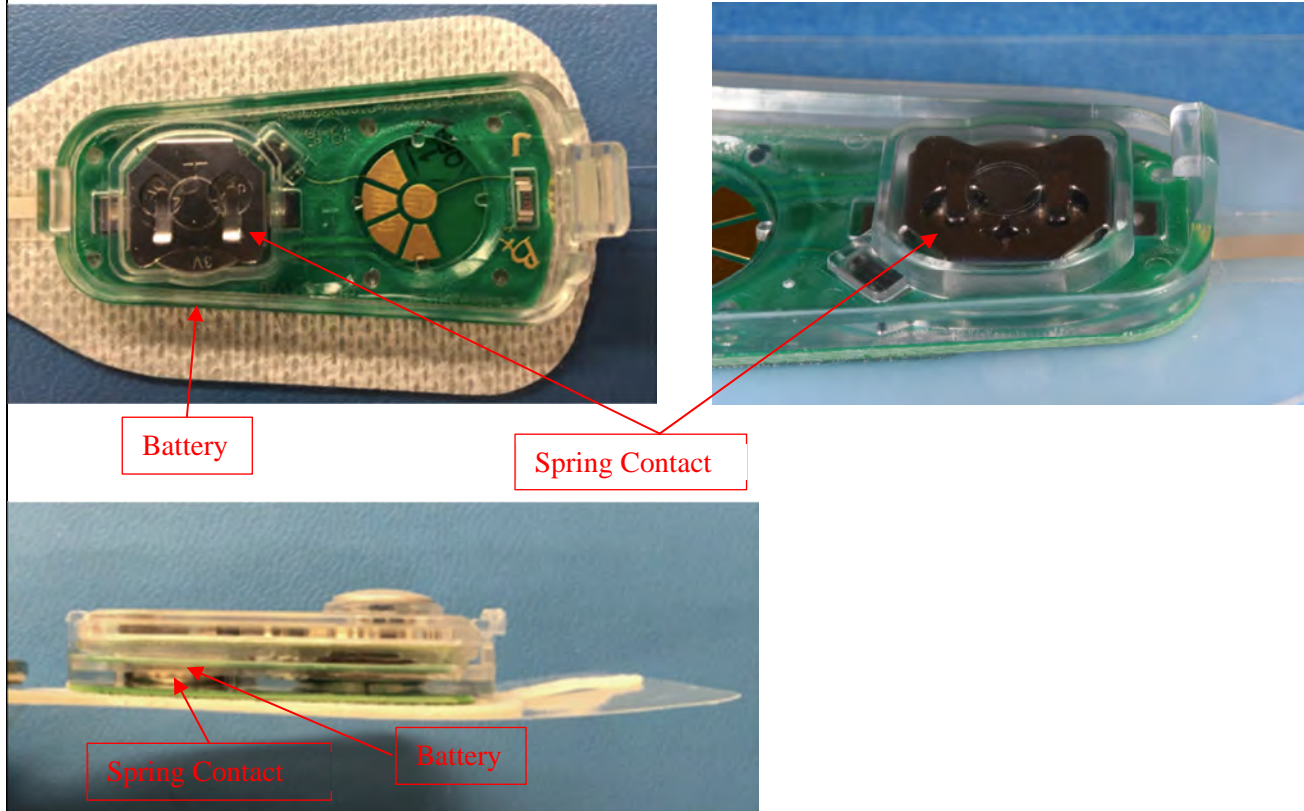

Alternatively, in another example, the Recorder of the Bardy CAM Patch product includes a spring contact. The spring contact on the Recorder is configured to electrically couple a battery to a circuit board assembly on the Recorder.

**Infringement of U.S. Patent No. 12,245,860
By the Bardy CAM Patch Product**



The Bardy CAM Patch product also comprises a circuit board assembly housed within the first housing portion.

**Infringement of U.S. Patent No. 12,245,860
By the Bardy CAM Patch Product**



Carnation Ambulatory Monitor

by Bardy Diagnostics

Designed to be placed along the sternum — over the heart — to optimize P-wave signal capture, the **CAM** Patch results in improved ECG clarity, providing more information about heart rhythm that may lead to more clinically-actionable diagnoses compared to leading ECG monitors in the industry. Its unique form factor is designed with comfort and satisfaction in mind, with the aim of improving patient compliance.¹⁻⁴

Event button to mark the continuous recording of patient symptoms

Proprietary circuit design enabling optimal signal-to-noise

Lightweight and low-profile design

Slim hourglass shape


Durable long-term adhesive suitable for sensitive skin

Image represents actual size of Carnation Ambulatory Monitor



<https://www.bardydx.com/wp-content/uploads/2022/12/DN000601A-14Day-Half-fold-CAM-Brochure.pdf>


**Infringement of U.S. Patent No. 12,245,860
By the Bardy CAM Patch Product**

	 <p data-bbox="611 228 804 313">Circuit Board Assembly</p> <p data-bbox="705 621 1003 678">First Housing Portion</p>
<p>[1.b] a flexible substrate coupled to a second housing portion, wherein the flexible substrate comprises a first layer and a second layer, and wherein the first layer extends beyond the second layer creating an edge to the flexible substrate that is thinner than an inner portion of the flexible substrate;</p>	<p>The Bardy CAM Patch product comprises a flexible substrate coupled to a second housing portion, wherein the flexible substrate comprises a first layer and a second layer, and wherein the first layer extends beyond the second layer creating an edge to the flexible substrate that is thinner than an inner portion of the flexible substrate.</p> <p>For example, the Bardy CAM Patch product includes a component that Bardy calls a Battrode, which includes a flexible substrate coupled to a second housing portion.</p>


**Infringement of U.S. Patent No. 12,245,860
By the Bardy CAM Patch Product**



(<https://youtube/RPcdb-volpc?si=meNXw98UDtIgwqp1&t=126>)

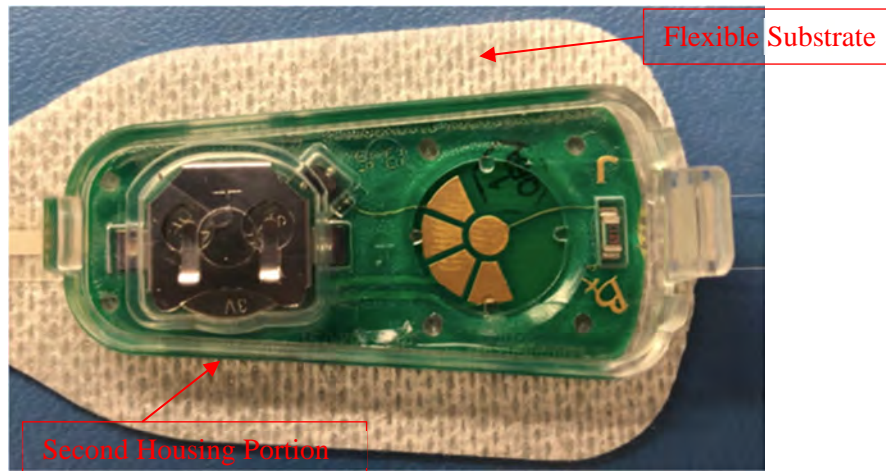


**Infringement of U.S. Patent No. 12,245,860
By the Bardy CAM Patch Product**

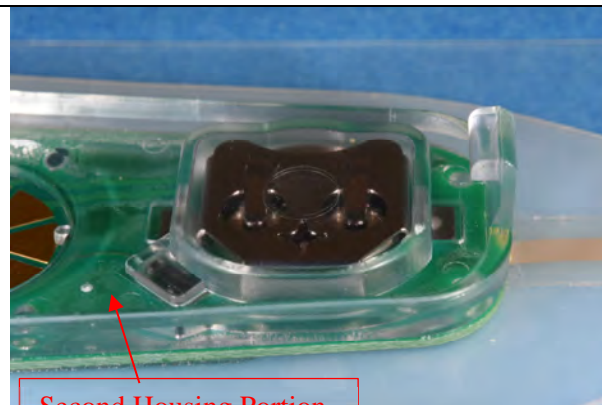

Second Housing Portion

For example, the Bardy CAM Patch product comprises wherein the flexible substrate comprises a first layer and a second layer. The image below shows a purple-colored area where the first and second layers overlap, in proximity to the electrode trace and electrode to the right.

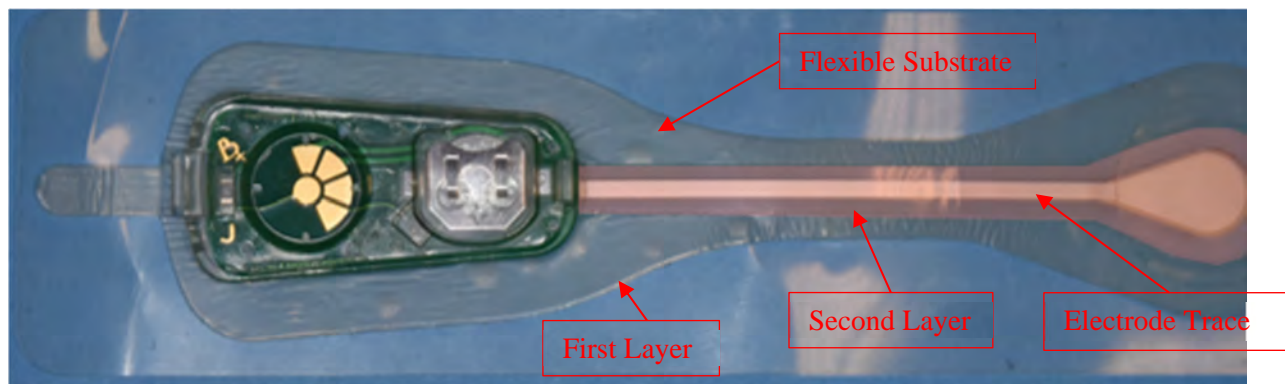

For example, the Bardy CAM Patch product also comprises wherein the first layer extends beyond the second layer creating an edge to the flexible substrate that is thinner than an inner portion of the flexible substrate. As shown in the image above, the second layer overlaps with the first layer in the purple-colored inner portion of the flexible substrate. Thus, the first layer extends beyond the second layer

**Infringement of U.S. Patent No. 12,245,860
By the Bardy CAM Patch Product**

	creating an edge to the flexible substrate that is thinner than the inner portion of the flexible substrate.
[1.c] an electrode coupled to the flexible substrate and configured to detect physiological signals of the patient to obtain the cardiac rhythm data;	<p>The Bardy CAM Patch product comprises an electrode coupled to the flexible substrate and configured to detect physiological signals of the patient to obtain the cardiac rhythm data.</p> <p>For example, the Bardy CAM Patch comprises an electrode coupled to the flexible substrate and configured to detect physiological signals of the patient to obtain the cardiac rhythm data.</p>

**Infringement of U.S. Patent No. 12,245,860
By the Bardy CAM Patch Product**



Carnation Ambulatory Monitor

by Bardy Diagnostics

Designed to be placed along the sternum — over the heart — to optimize P-wave signal capture, the **CAM Patch** results in improved ECG clarity, providing more information about heart rhythm that may lead to more clinically-actionable diagnoses compared to leading ECG monitors in the industry. Its unique form factor is designed with comfort and satisfaction in mind, with the aim of improving patient compliance.¹⁻⁴

Event button to mark the continuous recording of patient symptoms

Proprietary circuit design enabling optimal signal-to-noise

Lightweight and low-profile design

Slim hourglass shape

Durable long-term adhesive suitable for sensitive skin



Flexible Substrate

Electrode

Image represents actual size of Carnation Ambulatory Monitor

(<https://www.bardydx.com/wp-content/uploads/2022/12/DN000601A-14Day-Half-fold-CAM-Brochure.pdf>)

**Infringement of U.S. Patent No. 12,245,860
By the Bardy CAM Patch Product**

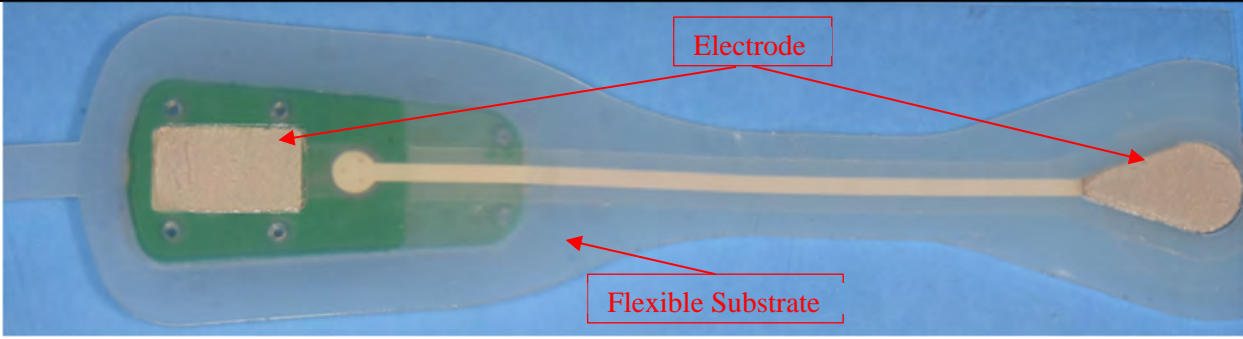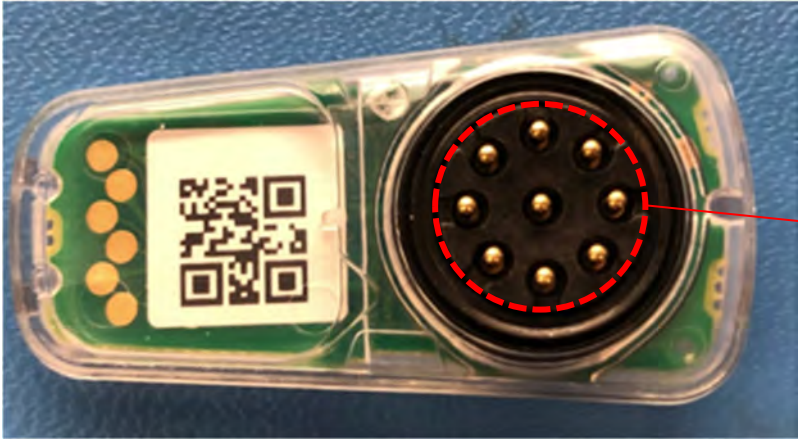	 <p>The diagram shows a top-down view of the Bardy CAM Patch product. It consists of a long, thin, light-colored flexible substrate. At one end, there is a larger, rectangular, light-colored electrode. At the other end, there is a smaller, oval-shaped electrode. A red arrow points from the label 'Electrode' to the larger rectangular electrode, and another red arrow points from the label 'Flexible Substrate' to the main body of the device.</p>
<p>[1.d] a support post configured such that force from interaction with a trigger is transmitted to the support post; and</p>	<p>The Bardy CAM Patch product comprises a support post configured such that force from interaction with a trigger is transmitted to the support post.</p> <p>For example, the Bardy CAM Patch product comprises gold support posts on the underside of the Recorder that receive a force when the trigger, called an Event Button, is pressed. As shown in the below images, the Bardy CAM Patch includes an Event Button located above the support posts.</p>  <p>The image shows a top-down view of the Bardy CAM Patch product, which is a small, rectangular device with a clear plastic cover. On the left side, there is a QR code. On the right side, there is a circular array of gold support posts. A red dashed circle highlights the support posts, and a red arrow points from the label 'Support Posts' to one of the posts.</p>

**Infringement of U.S. Patent No. 12,245,860
By the Bardy CAM Patch Product**



Support Posts



Trigger/Event Button

Support Posts
(underneath)

**Infringement of U.S. Patent No. 12,245,860
By the Bardy CAM Patch Product**



**Infringement of U.S. Patent No. 12,245,860
By the Bardy CAM Patch Product**


	<div data-bbox="583 256 655 321" data-label="Image"> </div> <div data-bbox="655 261 1289 339" data-label="Section-Header"> <h2>Carnation Ambulatory Monitor</h2> <p>by Bardy Diagnostics</p> </div> <div data-bbox="613 427 978 886" data-label="Text"> <p>Designed to be placed along the sternum — over the heart — to optimize P-wave signal capture, the CAM Patch results in improved ECG clarity, providing more information about heart rhythm that may lead to more clinically-actionable diagnoses compared to leading ECG monitors in the industry. Its unique form factor is designed with comfort and satisfaction in mind, with the aim of improving patient compliance.¹⁻⁴</p> </div> <div data-bbox="1024 370 1255 461" data-label="Text"> <p>Event button to mark the continuous recording of patient symptoms</p> </div> <div data-bbox="1024 485 1224 550" data-label="Text"> <p>Proprietary circuit design enabling optimal signal-to-noise</p> </div> <div data-bbox="1071 587 1224 631" data-label="Text"> <p>Lightweight and low-profile design</p> </div> <div data-bbox="1050 769 1224 792" data-label="Text"> <p>Slim hourglass shape</p> </div> <div data-bbox="997 956 1224 1000" data-label="Text"> <p>Durable long-term adhesive suitable for sensitive skin</p> </div> <div data-bbox="915 1032 1325 1052" data-label="Text"> <p><small>Image represents actual size of Carnation Ambulatory Monitor</small></p> </div> <div data-bbox="1268 233 1541 1068" data-label="Image"> </div> <div data-bbox="550 1114 1772 1185" data-label="Text"> <p>(https://www.bardydx.com/wp-content/uploads/2022/12/DN000601A-14Day-Half-fold-CAM-Brochure.pdf)</p> </div>
<p>[1.e] a flexible electrode trace coupled to the flexible substrate and configured to electrically couple the electrode to the</p>	<p>The Bardy CAM product comprises a flexible electrode trace coupled to the flexible substrate and configured to electrically couple the electrode to the circuit board assembly, wherein at least a portion of the flexible electrode trace is in electrical contact with a second spring contact, and wherein the second spring contact is further configured to electrically couple the flexible electrode trace to the circuit board</p>

**Infringement of U.S. Patent No. 12,245,860
By the Bardy CAM Patch Product**

circuit board assembly, wherein at least a portion of the flexible electrode trace is in electrical contact with a second spring contact, and wherein the second spring contact is further configured to electrically couple the flexible electrode trace to the circuit board assembly.

assembly.


For example, the Bardy CAM Patch product comprises a flexible electrode trace coupled to the flexible substrate and configured to electrically couple the electrode to the circuit board assembly.

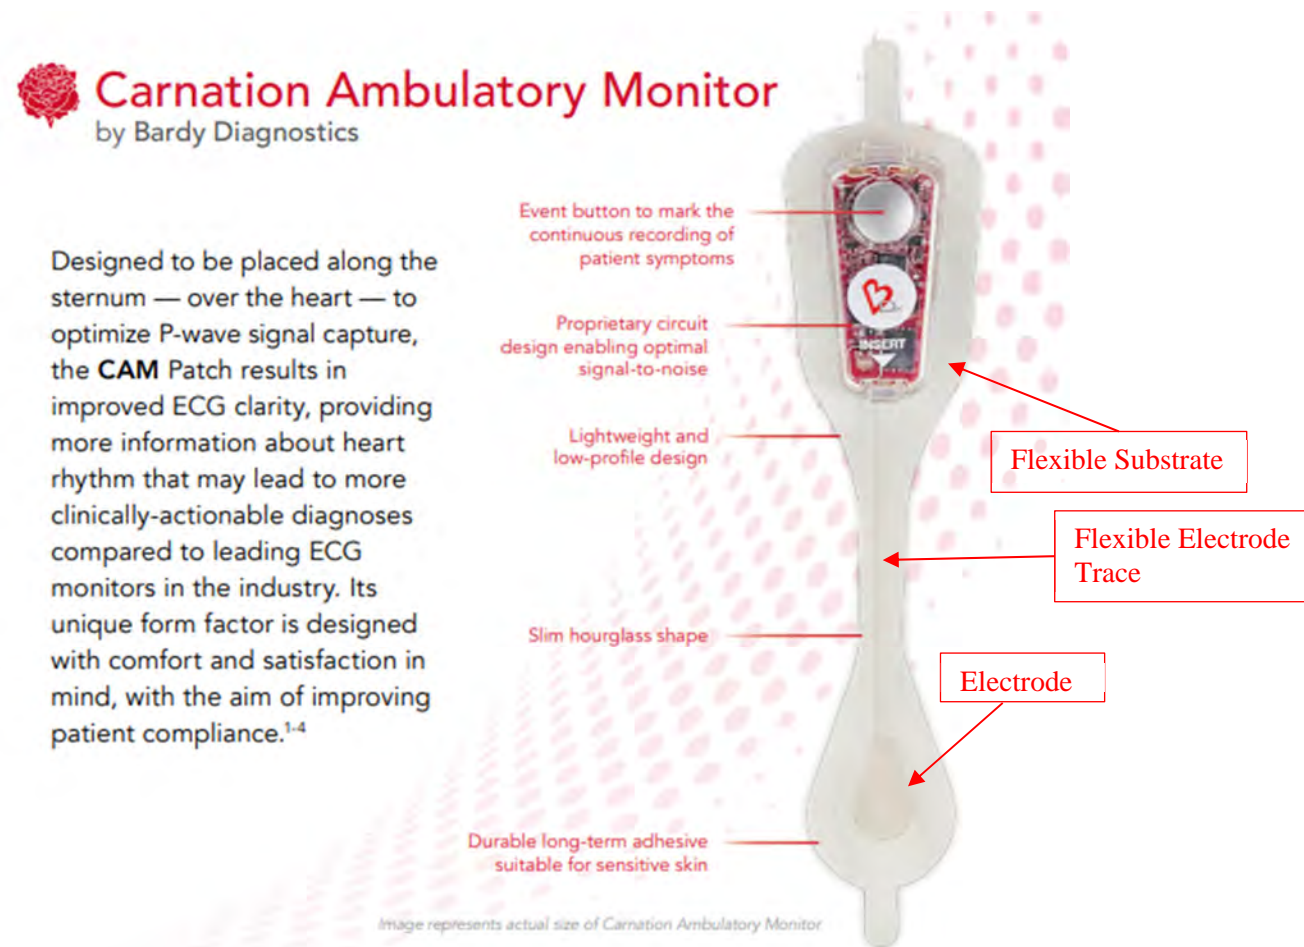

(<https://www.bardydx.com/wp-content/uploads/2022/12/DN000601A-14Day-Half-fold-CAM->

**Infringement of U.S. Patent No. 12,245,860
By the Bardy CAM Patch Product**


[Brochure.pdf](#))

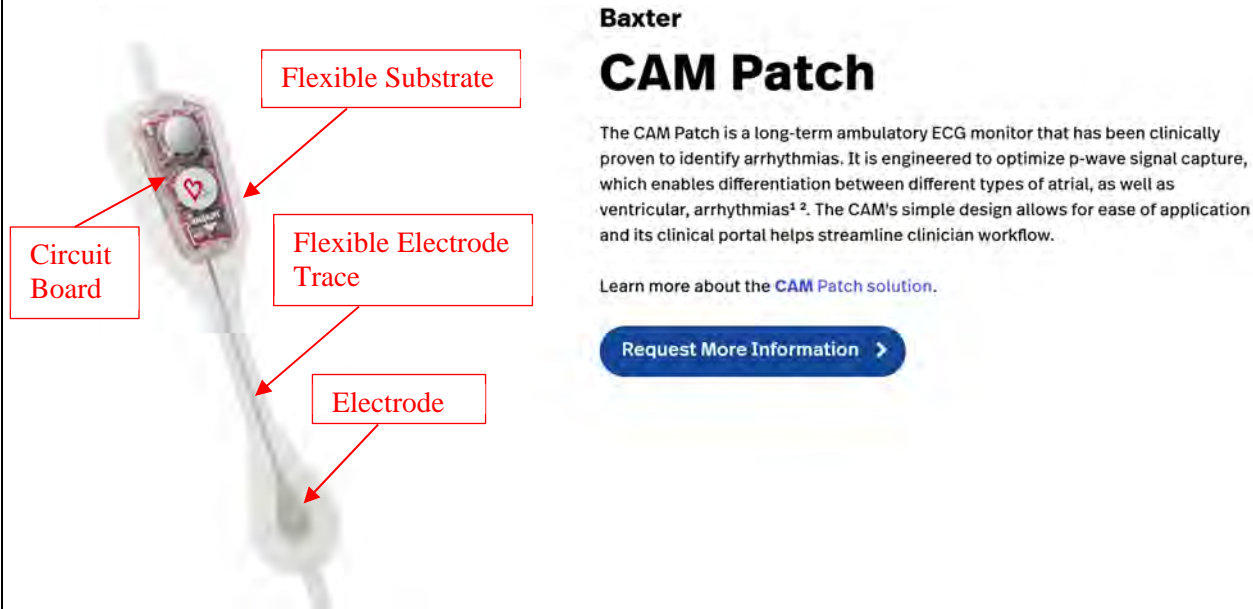

(<https://www.hillrom.com/en/products/cam-patch/>)

For example, the Recorder of the Bardy CAM patch comprises a second spring contact. At least a portion of the flexible electrode trace is in electrical contact with the second spring contact through the Battrode. This electrical connection allows the Recorder to receive signals from the flexible electrode trace.

**Infringement of U.S. Patent No. 12,245,860
By the Bardy CAM Patch Product**

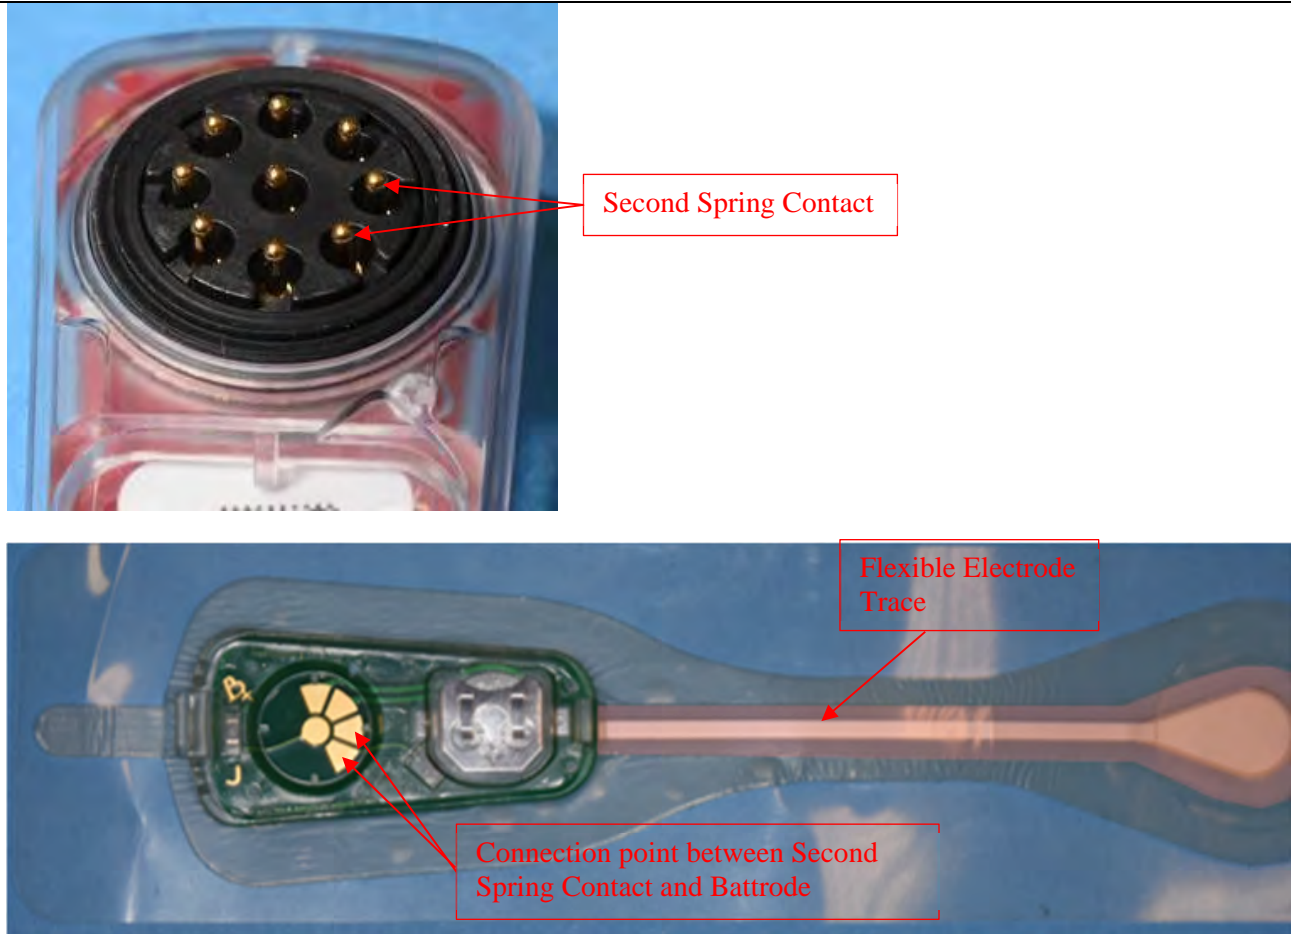


For example, the second spring contact of the Bardy CAM patch electrically couples the flexible electrode trace to the circuit board assembly. This electrical coupling allows the circuit board assembly on the Recorder to receive signals from the flexible electrode trace.

**Infringement of U.S. Patent No. 12,245,860
By the Bardy CAM Patch Product**



**Infringement of U.S. Patent No. 12,245,860
By the Bardy CAM Patch Product**

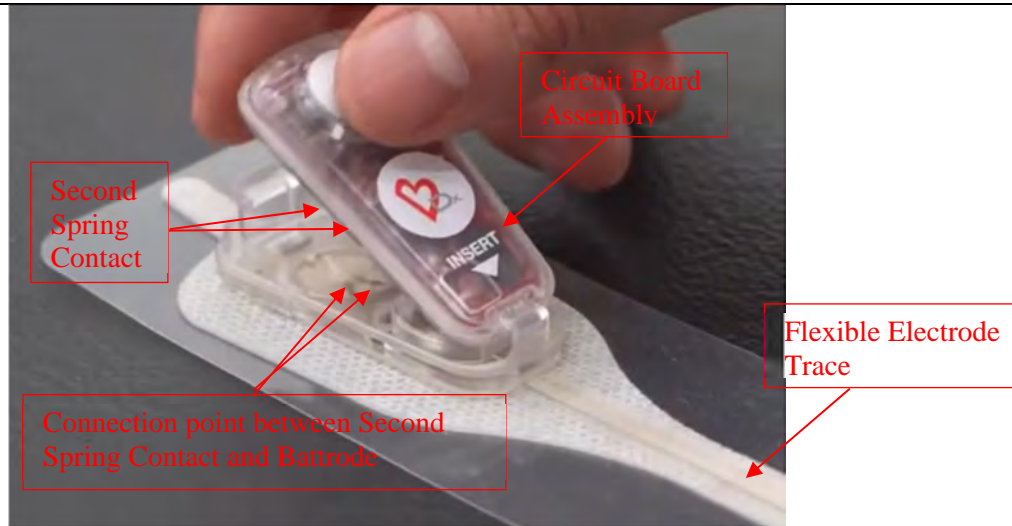

(<https://youtube/RPcdb-volpc?si=V-ITnQOLgrOrtUVa&t=119>)